




Erythromycin Gastro-resistant Tablets – BP 2021

These chromatograms are provided for information only as an aid to analysts and are intended as guidance for the interpretation and application of BP monographs.


Typical chromatogram for solution (3) in the Related Substances test for Erythromycin Gastro-resistant Tablets as published in BP 2021.

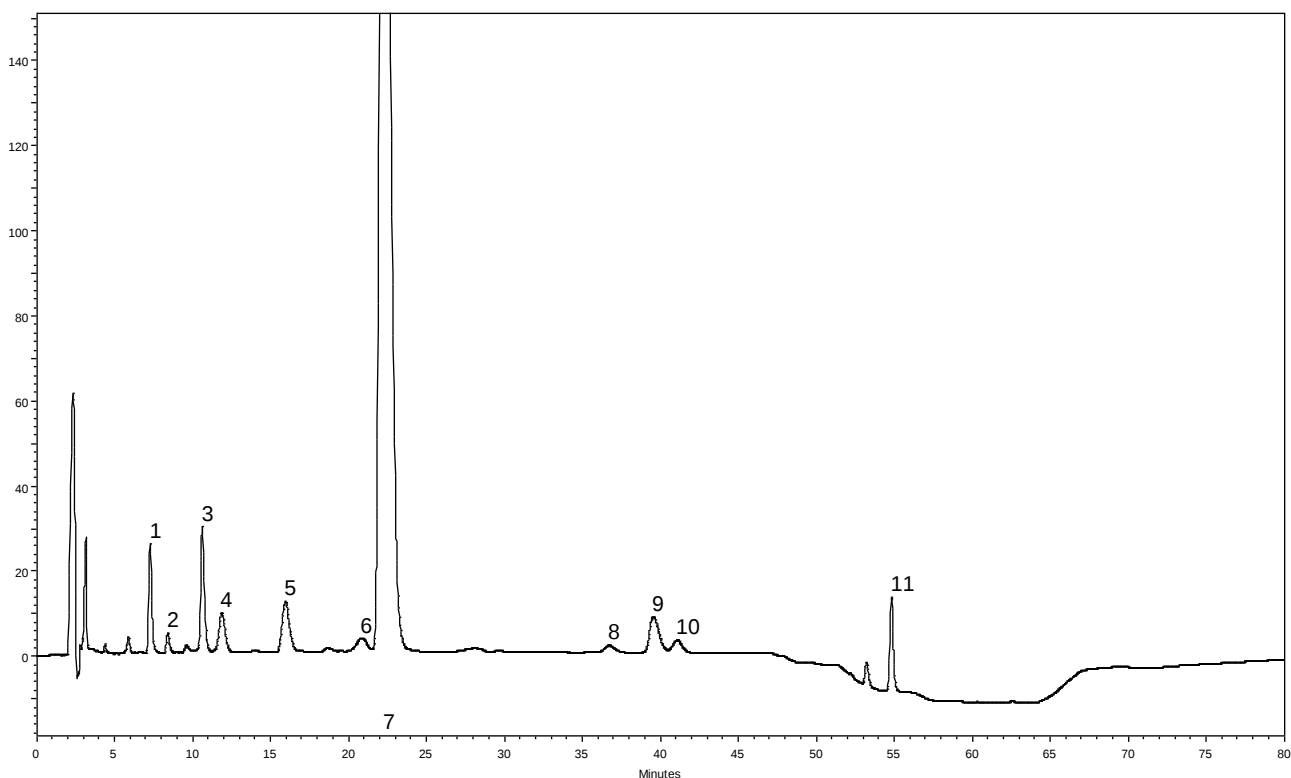

Peak ID: 1: Impurity H; 2: Impurity A; 3: Impurity B; 4: Erythromycin C; 5: Impurity L; 6: Impurity C; 7: Erythromycin A; 8: Impurity D; 9: Erythromycin B; 10: Impurity F; 11: Impurity E




Typical chromatogram for solution (4) in the Related Substances test for Erythromycin Gastro-resistant Tablets as published in BP 2021.

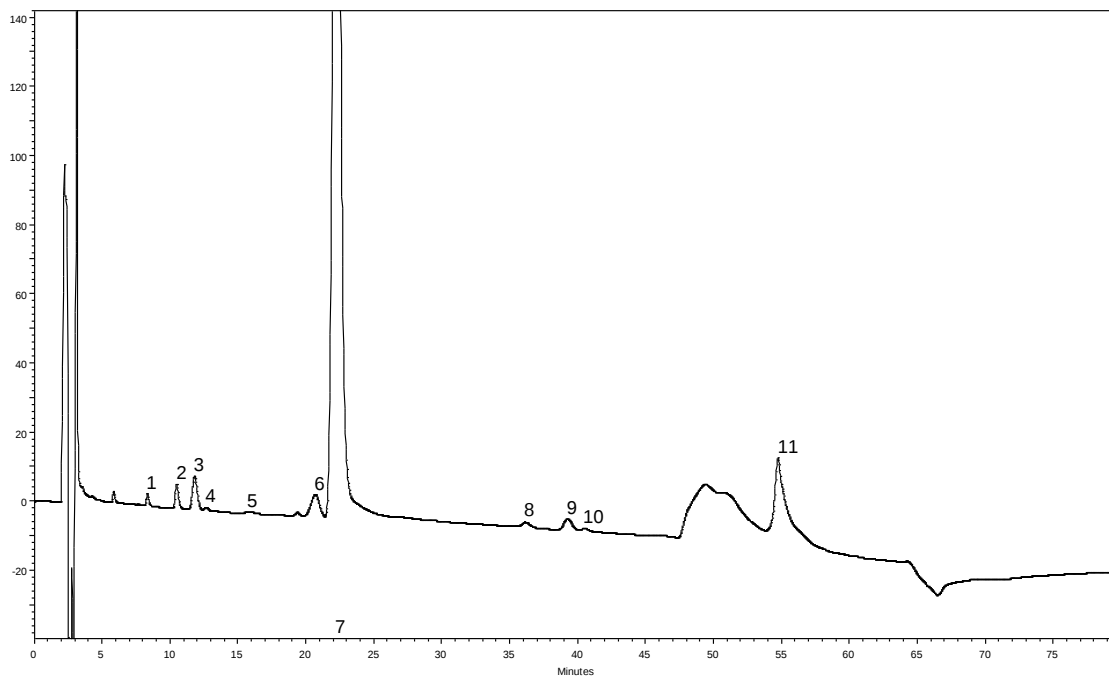

Peak ID: 1: Impurity A; 2: Impurity B; 3: Erythromycin C; 4: Impurity M; 5: Impurity L; 6: Impurity C; 7: Erythromycin A; 8: Impurity D; 9: Erythromycin B; 10: Impurity F; 11: Impurity E


Typical chromatogram for solution (2) in the Assay test for Erythromycin Gastro-resistant Tablets as published in BP 2021.

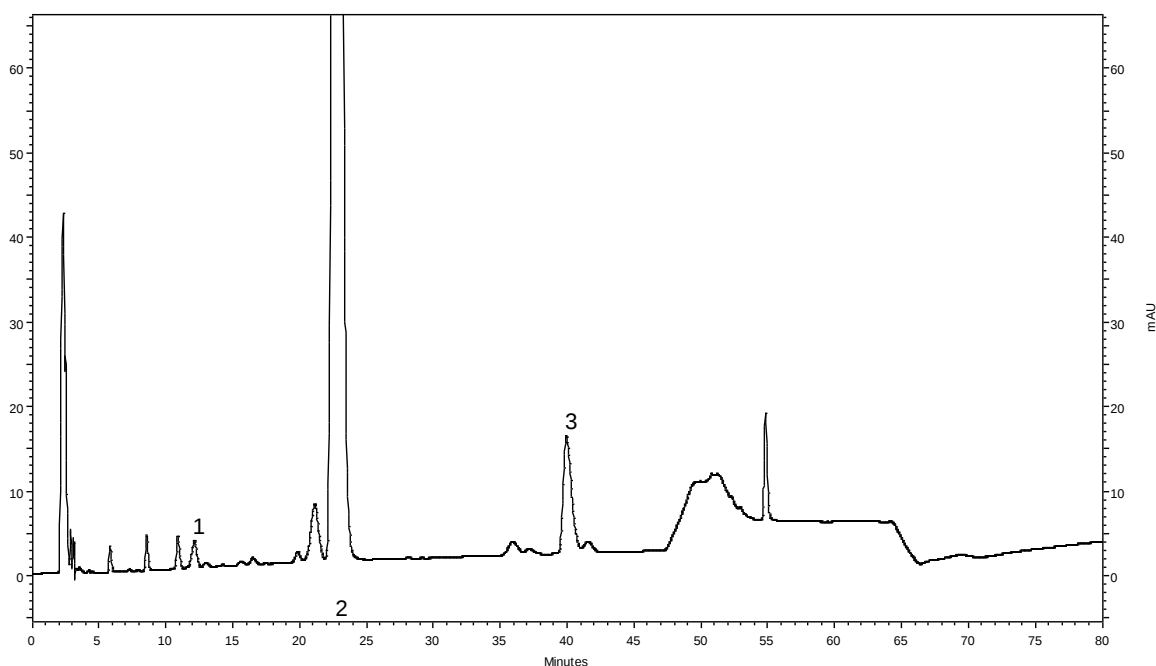

Peak ID: 1: Erythromycin C; 2: Erythromycin A; 3: Erythromycin B



Typical chromatogram for solution (3) in the Assay test for Erythromycin Gastro-resistant Tablets as published in BP 2021.

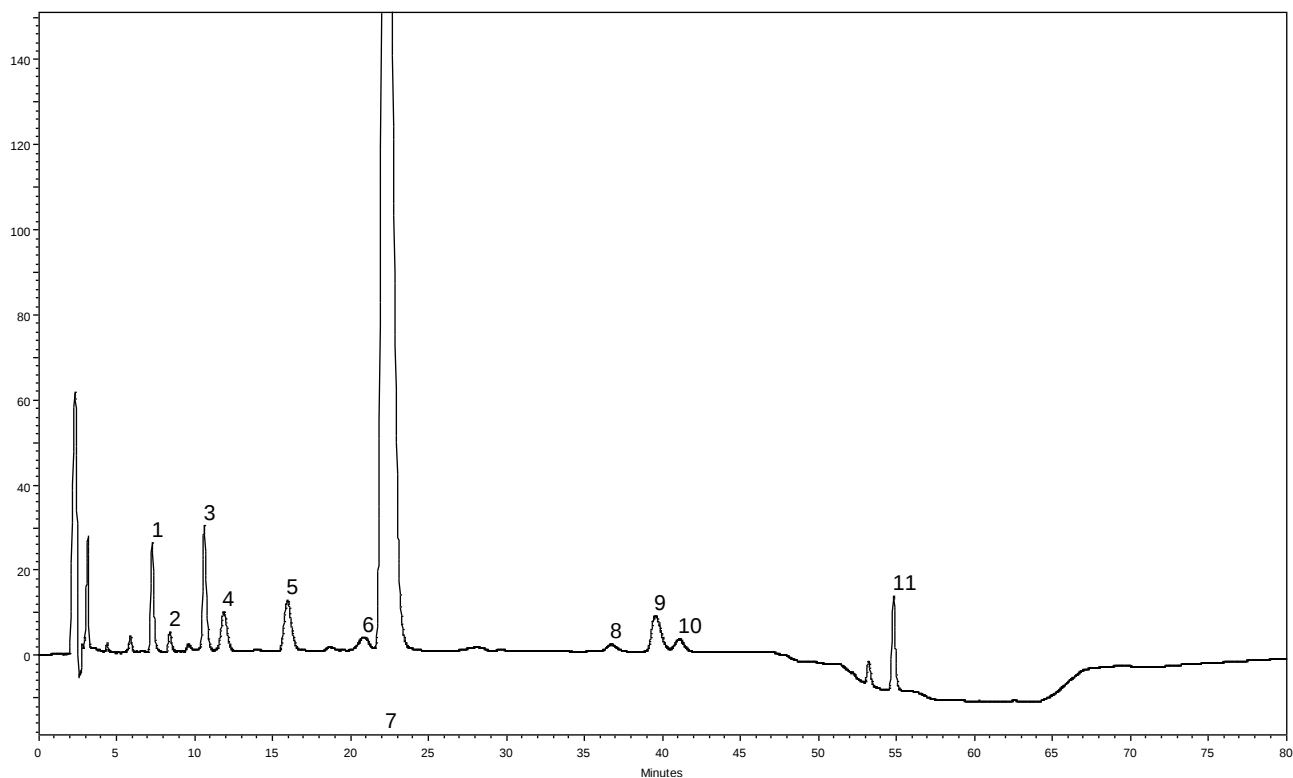

Peak ID: 1: Impurity H; 2: Impurity A; 3: Impurity B; 4: Erythromycin C; 5: Impurity L; 6: Impurity C; 7: Erythromycin A; 8: Impurity D; 9: Erythromycin B; 10: Impurity F; 11: Impurity E

Column : XTerra RP18 (250 mm x 4.6 mm, 3.5 μ m)
Method Ref. : Assay for the Erythromycin Gastro-resistant Tablets monograph from BP 2021
Mobile Phase A : Buffer: acetonitrile: water (5: 35: 60, v/v/v)
Mobile Phase B : Buffer: water: acetonitrile (5: 45: 50, v/v/v)
Buffer : 3.5 % w/v dipotassium hydrogen phosphate adjusted to pH 7.0 with dilute phosphoric acid
Diluent : 1.15 % w/v dipotassium hydrogen phosphate adjusted to pH 8.0 with orthophosphoric acid: methanol (40: 60, v/v)

Gradient		<table><tr><th>Time (min)</th><th>Mobile Phase A (%)</th><th>Mobile Phase B (%)</th></tr><tr><td>0-44</td><td>100</td><td>0</td></tr><tr><td>44-46</td><td>100-0</td><td>0-100</td></tr><tr><td>46-61</td><td>0</td><td>100</td></tr><tr><td>61-63</td><td>0-100</td><td>100-0</td></tr><tr><td>63-80</td><td>100</td><td>0</td></tr></table>	Time (min)	Mobile Phase A (%)	Mobile Phase B (%)	0-44	100	0	44-46	100-0	0-100	46-61	0	100	61-63	0-100	100-0	63-80	100	0
Time (min)	Mobile Phase A (%)	Mobile Phase B (%)																		
0-44	100	0																		
44-46	100-0	0-100																		
46-61	0	100																		
61-63	0-100	100-0																		
63-80	100	0																		

Flow rate : 1.0 mL/min
Column Temp : 65 °C
Injection Volume : 100 μ L
Detection : 210 nm