




Oxycodone Injection – BP 2016


These chromatograms are provided for information only as an aid to analysts and intended as guidance for the interpretation and application of BP monographs.

Typical chromatogram for solution (4) in the Related substances test for Oxycodone Injection as published in BP 2016.

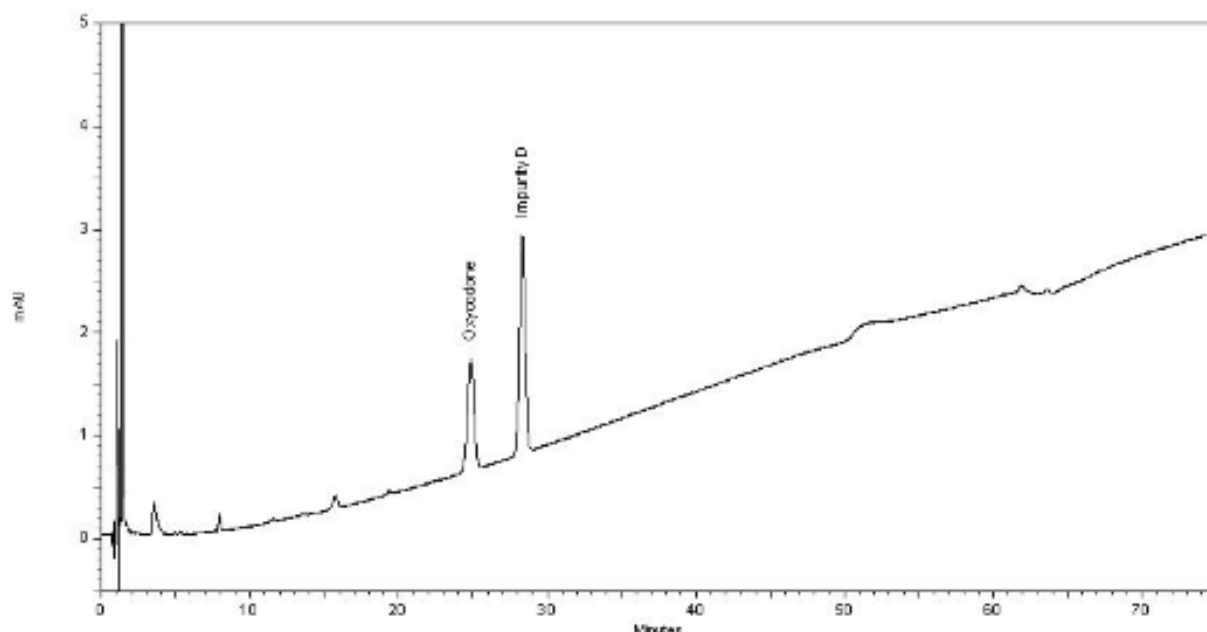

The chromatogram shows two peaks oxycodone (<2 mAU) at 24.8 minutes and impurity D (<3 mAU) at 28.3 minutes.

Typical chromatogram for solution (1) in the Related substances samples test for Oxycodone Injection as published in BP 2016.

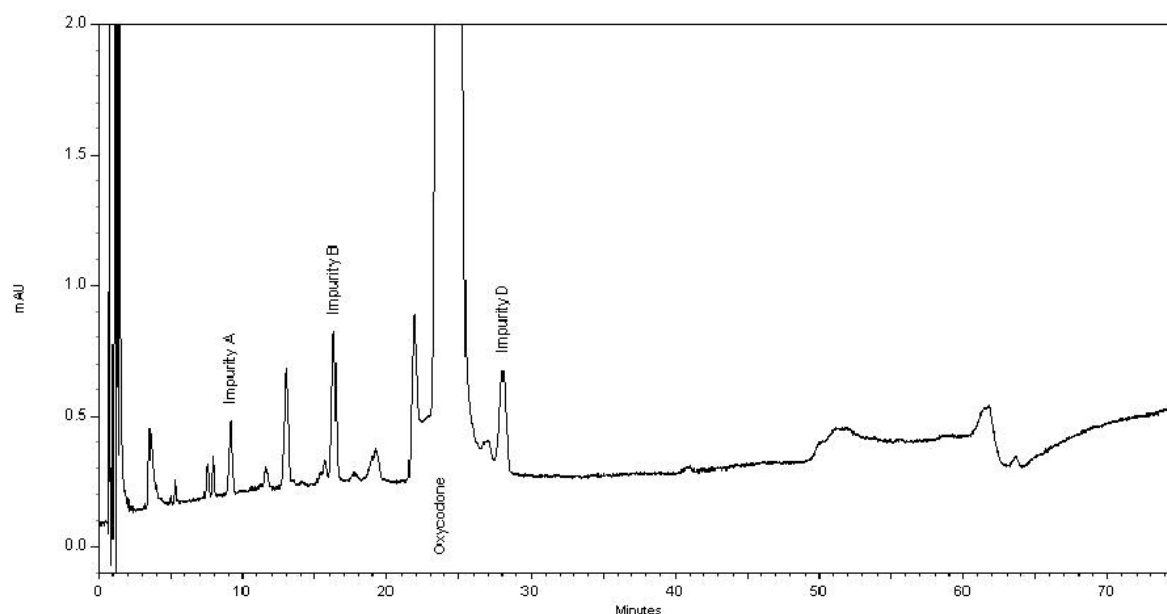

The chromatogram shows a large oxycodone peak (off scale at 2 mAU) at 23.8 minutes and three known peaks, impurity A (<1 mAU) at 9.2 minutes, Impurity B (<1 mAU) at 16.4 minutes, impurity D (<1 mAU) at 28.2 minutes.